


Figure 1



Received
08/01/03
2:15 PM



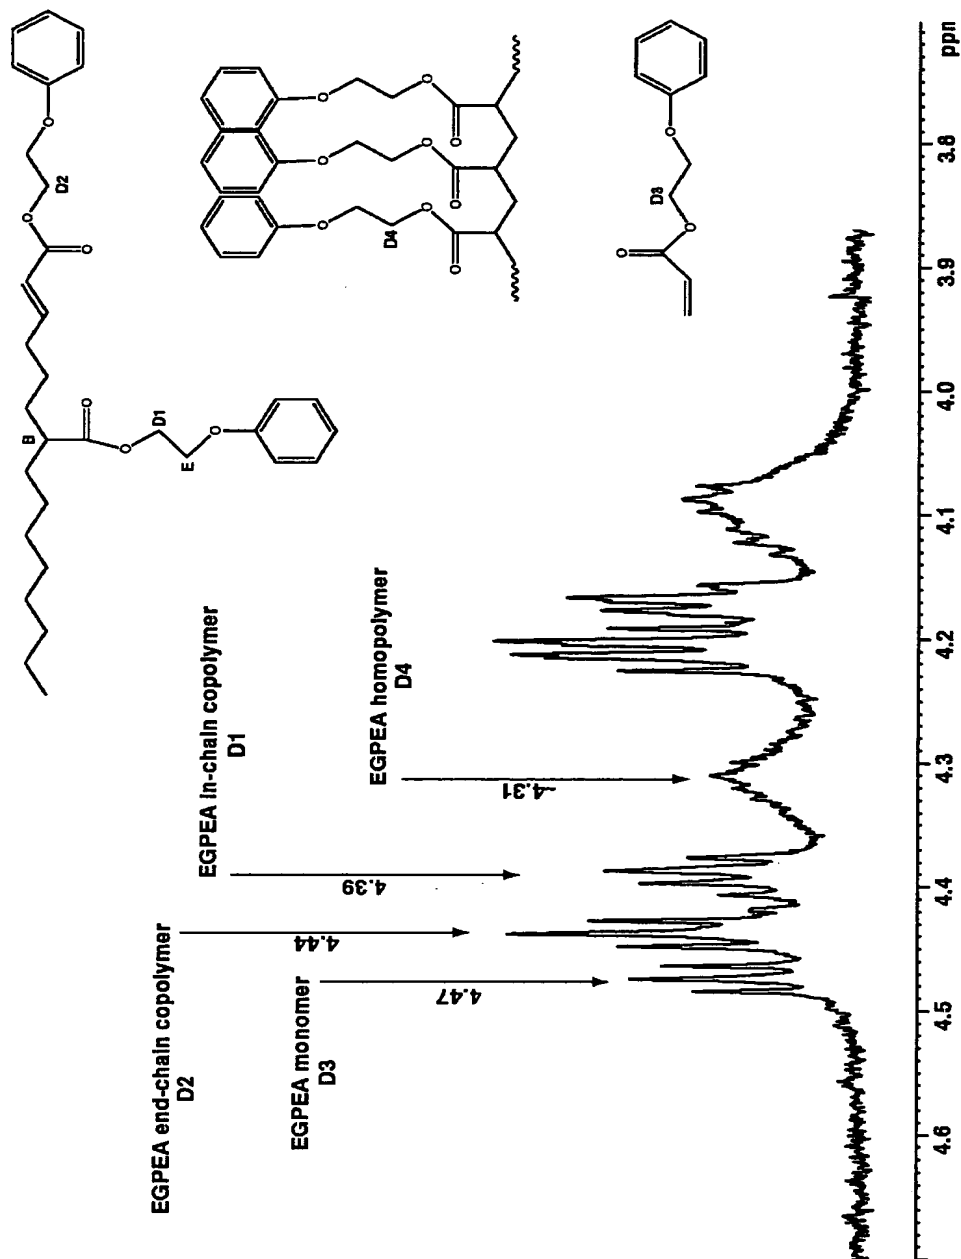

REVIEWED
2005 01 06
JMT/ST

310mg sample and 80 mg CrAcAc in total vol 3.1 ml TCB
Varian Unity 400 NMR Spectrometer
gea4 10mm probe, 120C, a locked, 13C NMR
DuPont NMR Lab E302/118

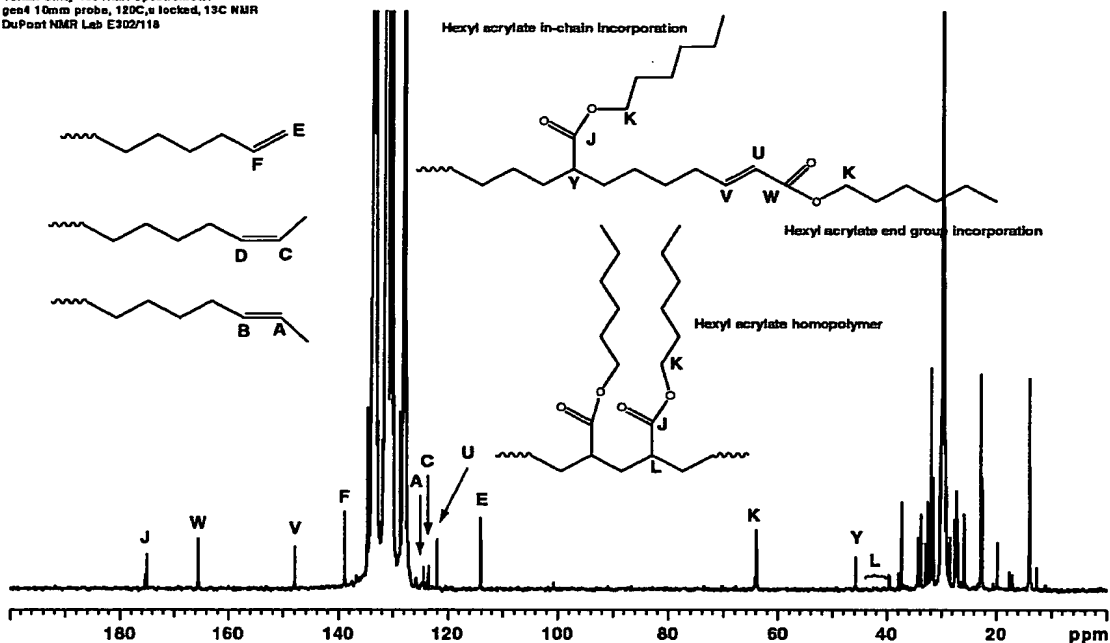


Figure 2

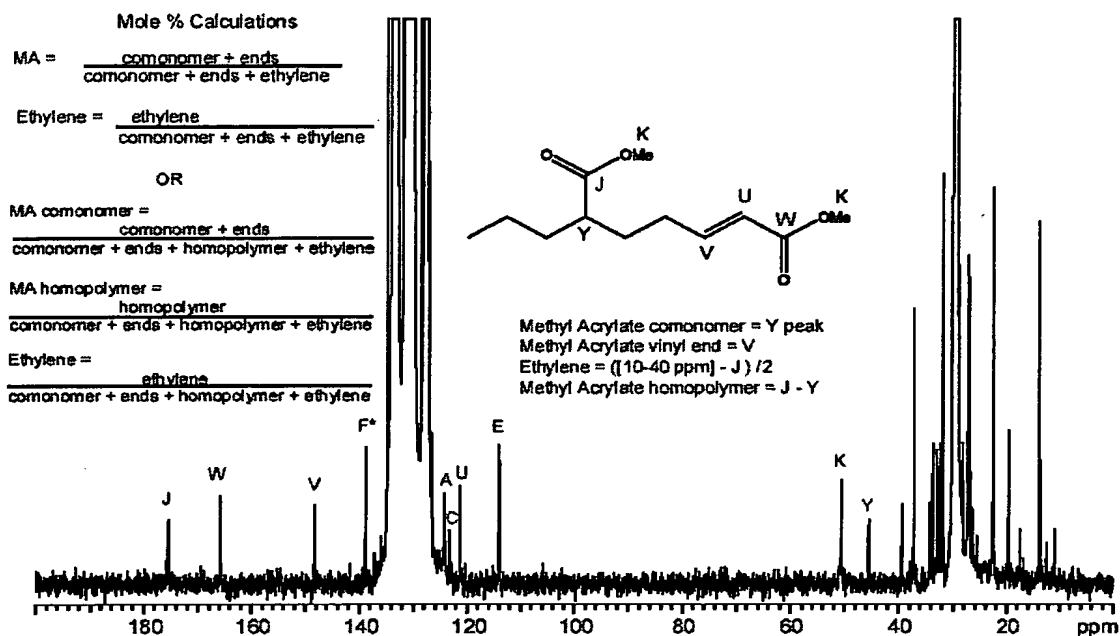


Figure 3